



# TEST REPORT


## FL900 Composite Cover Air BP Specification BS EN124 Class F900 Load Test

**Cover weight: 109.0kg**

Document reference number – FIB-FL900-AirBP-F900-01-04-25

**Report by:**

M.A.Salisbury  
Senior Technician

M. A. Salisbury 

**Date test carried out:**

1<sup>st</sup> April 2025

**Customer name:**

Fibrelite Composites Ltd.  
Snaygill Industrial Estate,  
Keighley Road,  
Skipton,  
North Yorkshire  
BD23 2QR


## Clarifying Statements:

1. The results reported have been performed in accordance with the test requirements agreed by the customer (Fibrelite Ltd.) and laid down in the new BS EN 124-1: 2015 standard, along with the composite section EN 124-5, plus the added criteria in the Air BP test specification.
2. This report does not include or imply any expert opinions as to the serviceability of the sample tested or their suitability for a specific purpose.
3. The submitter disclaims any liability of any kind for any damage whatsoever resulting from the use of either data in the files or the attached values of the test results reported.
4. The report may not be reproduced other than in full, except with the prior written consent of the Engineering Dept., Lancaster University.
5. All testing has been carried out in within the Engineering Department, Gillow Ave., Lancaster University, Bailrigg, Lancaster LA1 4YW.
6. This report applies only to those items and/or materials that have been tested and reported on herein. No inference shall be made to similar test items or materials/ samples.

## **Cover**

The composite cover supplied for testing is a square FL900 and comes complete with an aluminium frame. (Fig.1)


A 100mm x 100mm steel box section frame was placed over the unit to add extra support to the frame. Fig.1

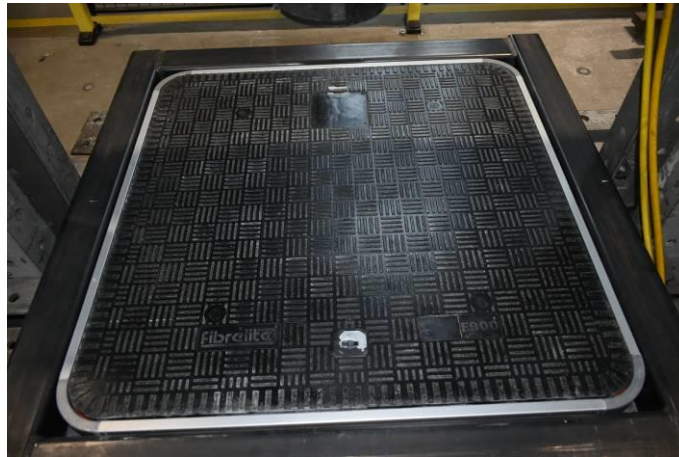

**Fig.1**

## **Test Rig**

The test rig consists of a 'giant mecano' frame bolted to the floor and supporting twin Enerpac 60 ton hydraulic cylinders. (Fig.2)

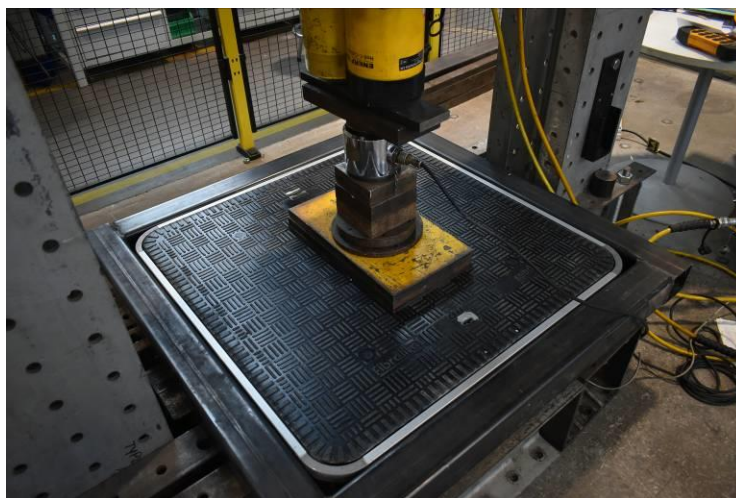

**Fig.2**

In accordance with the EN124-1:2015 standard the load cell and test rig complies with EN ISO 7500-1:2004 minimum Class 3.

System I.D.: TR150-17182835


Load Cell ID: NCB/MRE-440/3243

Instron Calibration Certificate No. E187070224093831

Calibrated on 2<sup>nd</sup> July 2024

System Class: 0.5

Figure 3 below shows the calibration certificate for the load cell and test rig.

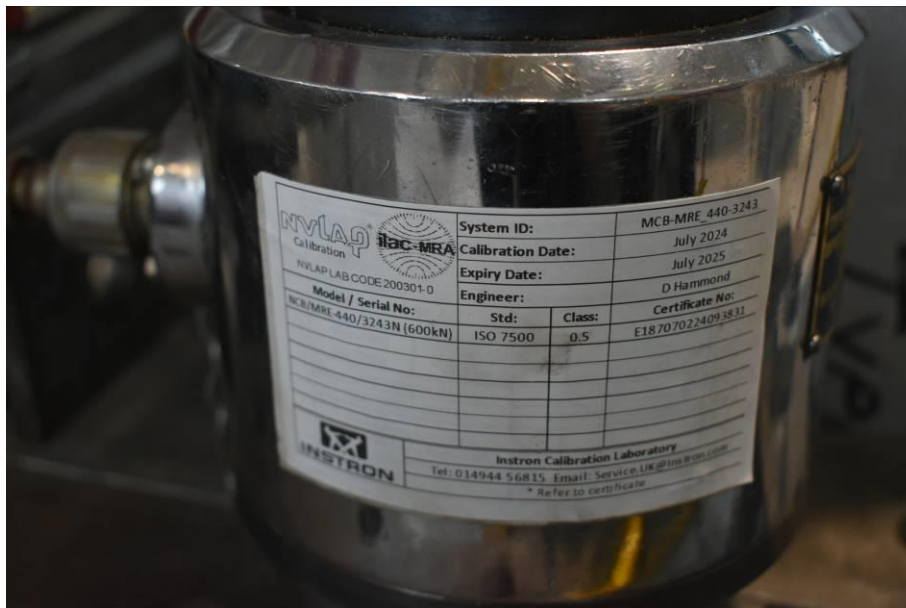

**Fig.3**

## **Test**

The tests were carried out in accordance with the BS EN124:2015 but with the added Air BP specification for:

- Permanent Set – Clause 8.2
- Load Bearing Capacity – Clause 8.3

**The loading pad used for the Air BP criteria is 476mm x 270mm which equates to 1285cm<sup>2</sup> which is within the 1300cm<sup>2</sup> allowed.**

**A 10mm rubber pad was used between cover and loading pad.**

### **Permanent Set Test**

Measurement of permanent set shall be made on the upper-side of the cover in the same place as the applied load at the longest dimension which can be inscribed within the cover through the centre point of the load application. The measurement device shall be positioned as close as possible to the centre point of the load application and the seating of the measuring device support as close as possible to the edge of the cover but not exceeding 10mm from the edge.

An initial reading is to be taken at the geometric centre of the cover before the first load or any preloading has taken place.

The load is then to be applied at a rate of 1kN/s to 5kN/s up to 2/3 of the test load. This procedure is to be carried out five times without significant disruption.

A final deflection reading shall then be taken and the permanent set determined as the difference of the measured readings between the first and fifth readings.

### **Load Bearing Capacity**

Immediately after the permanent set test the cover shall be loaded up to the test load at a rate of 1kN/s to 5kN/s.

The test load shall then be maintained for  $30_{-0}^{+2}$  seconds.

## Results

### Permanent set test



**Fig.4**

Initial Reading	0.00mm
Reading after 5 cycles	1.74mm
<b>Permanent Set</b>	<b>1.74mm</b>

Permissible permanent set for a F900 test is  $\frac{CO}{300} = 900/300 = 3.00\text{mm}$

**Therefore cover passes the permanent set test.**

## Load Bearing Capacity Test


Load applied immediately after the permanent set test.

Although the standard does not require it for the load bearing test, a measuring device (linear potentiometer) was placed on the underside of the cover directly under the loading point and deflection readings taken every 600kN for the five cycles and 50kN intervals after that.

## Results

LOAD (kN)	DEFLECTION (mm)	REMARKS
0	0.00	
600	17.02	
0	1.56	
600	17.16	
0	1.87	
600	17.51	
0	1.90	
600	17.45	
0	1.94	
600	17.69	
0	2.14	
50	3.60	
100	5.15	
150	6.69	
200	7.84	
250	9.20	
300	10.49	
350	11.59	
400	12.93	
450	14.14	
500	15.08	
550	16.33	
600	17.52	
650	19.05	
700	20.60	
750	22.13	
800	24.16	
850	27.09	
900	29.67	
900(10 seconds)	29.99	
900(20 seconds)	30.35	
900(30 seconds)	30.67	<b>PASS</b>
0	3.74	

**Fig.5**

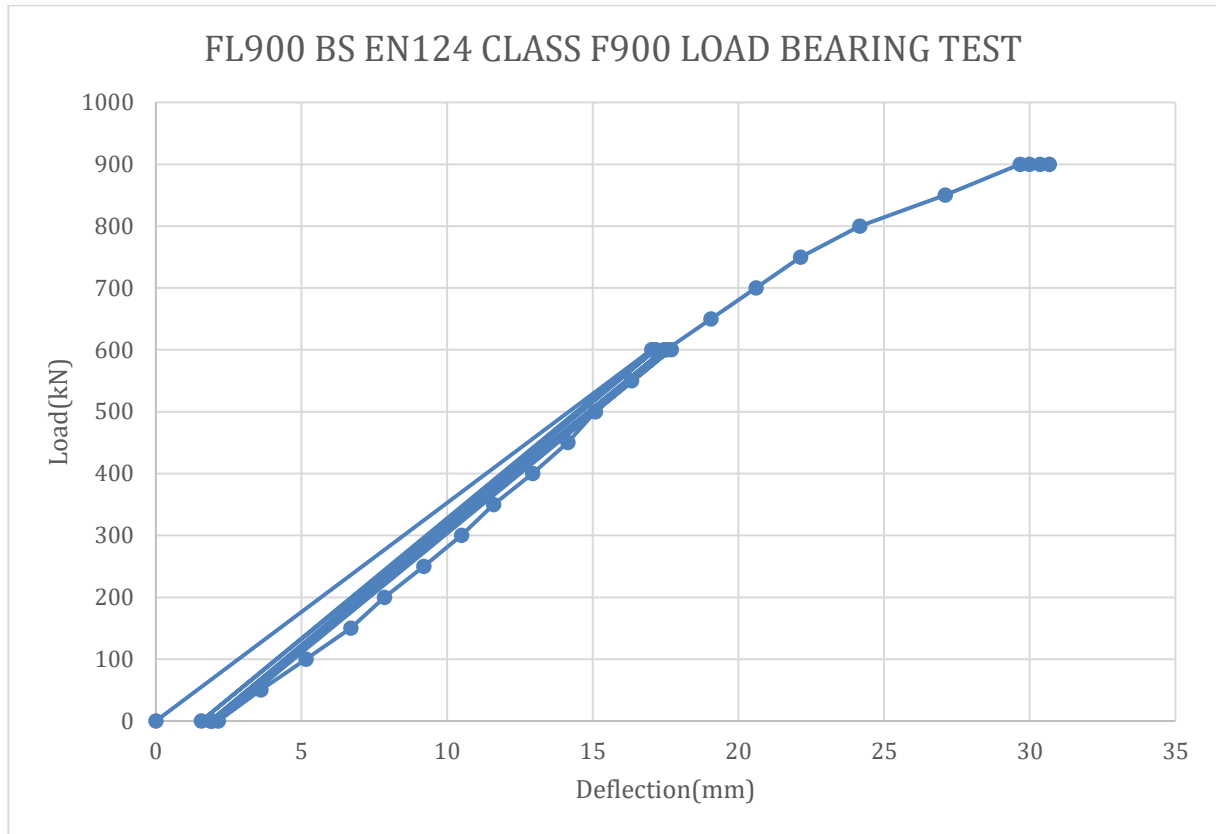

**Fig.6**

**The FL900 cover held the test load of 900kN for the required 30 seconds with no visible signs of damage, so therefore the cover passed BS EN124 Air BP Specification F900 load bearing test.**